


X-ray of Jodi Rouviere 8/14/2012 (Dr. Robert Buly)

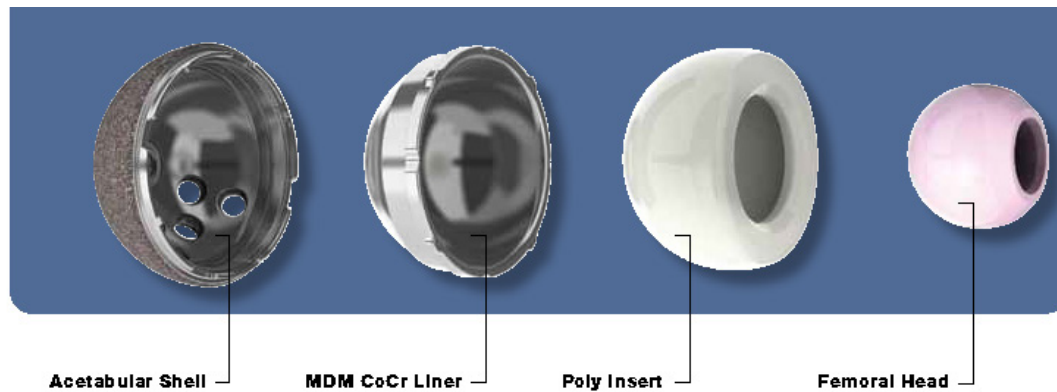


Acetabular Shell

MDM CoCr Liner

Poly Insert

Femoral Head

(Stryker MDMX3 Surgical Technique Brochure, pg 1)

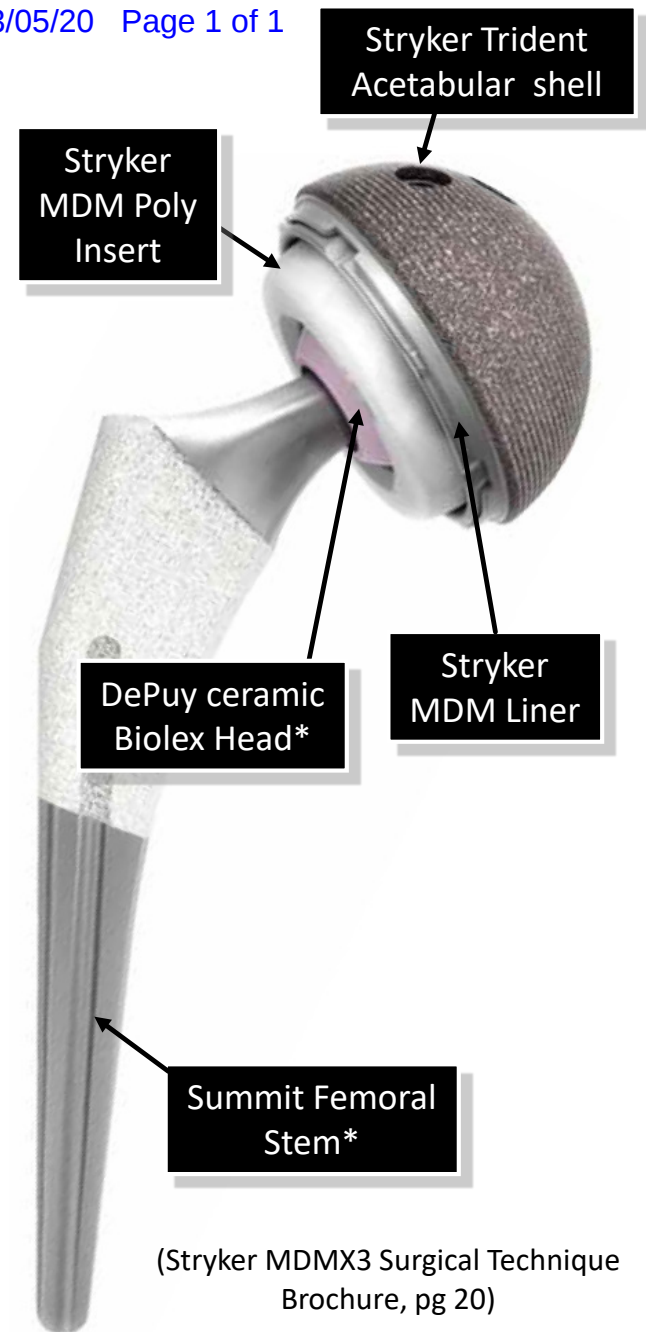

(Stryker MDMX3 Surgical Technique Brochure, pg 20)

*Exemplar of Plaintiffs' Device(s)